

1/15

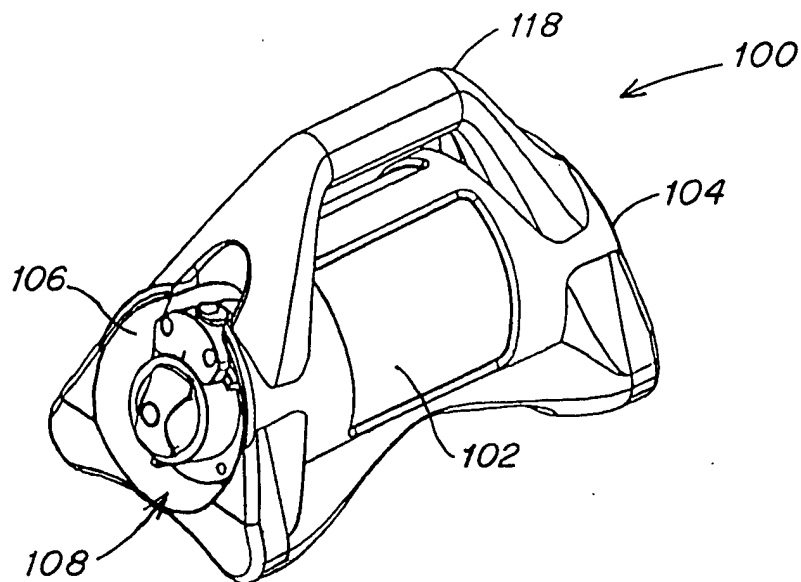


FIG. 1

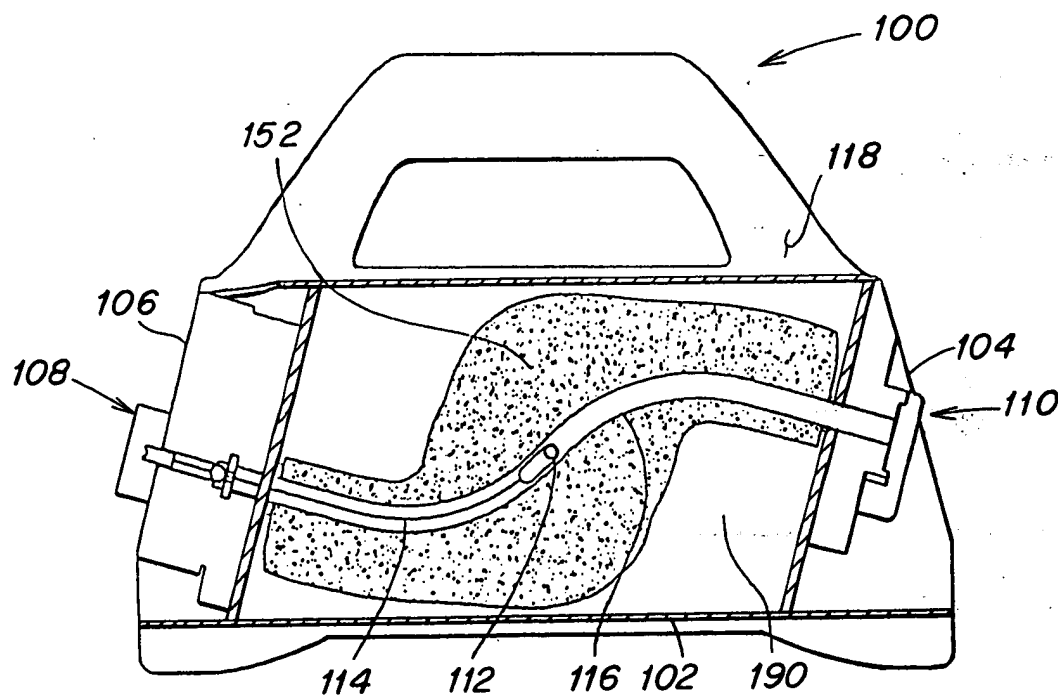


FIG. 2

2/15

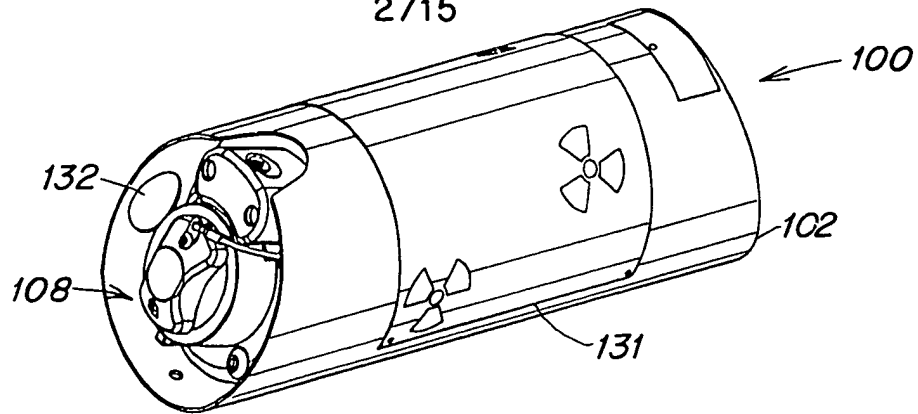


FIG. 3

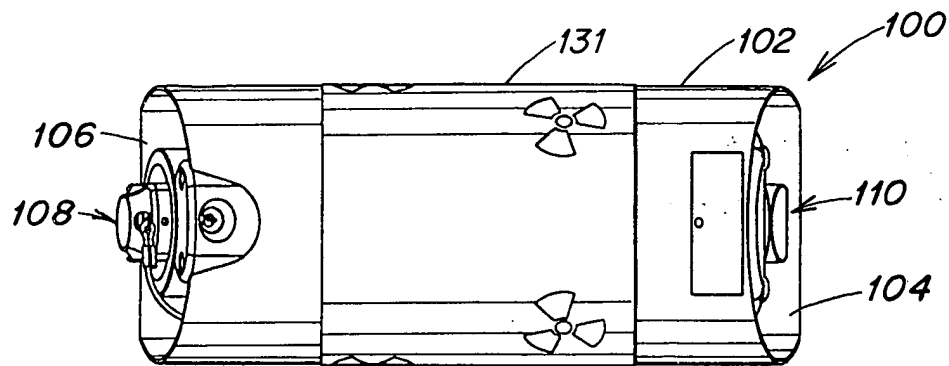


FIG. 4

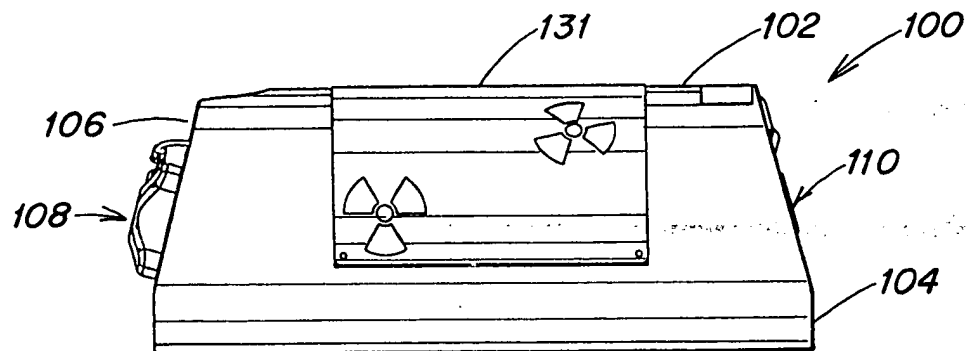


FIG. 5

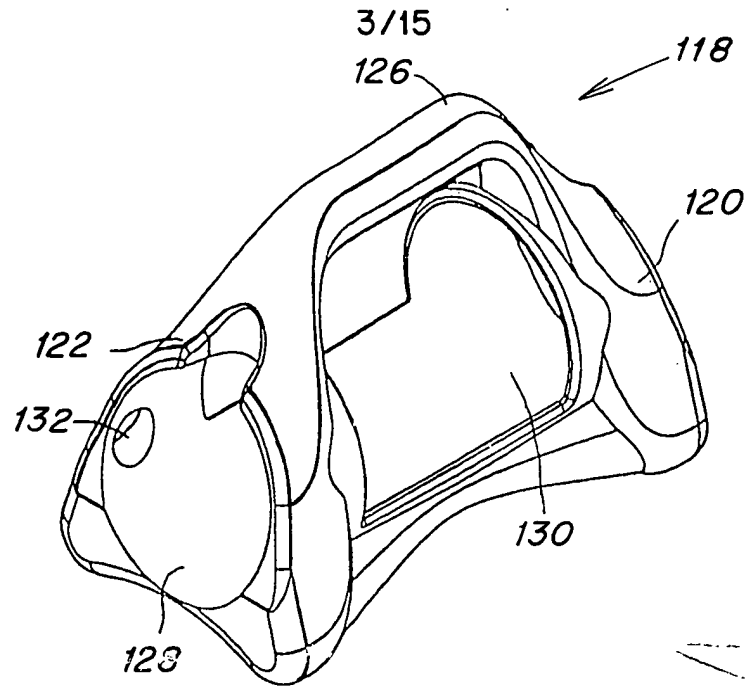


FIG. 6

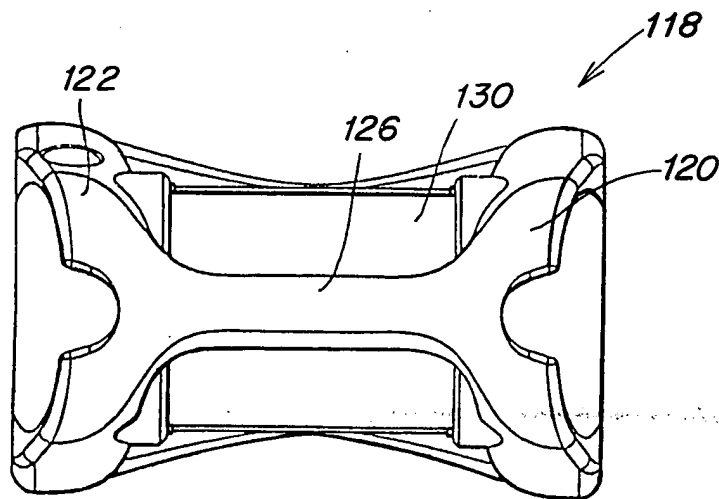


FIG. 7


**RADIOGRAPHIC CAMERA**

Steven J. Grenier


09/687,554

Sheet 4 of 15

4/15

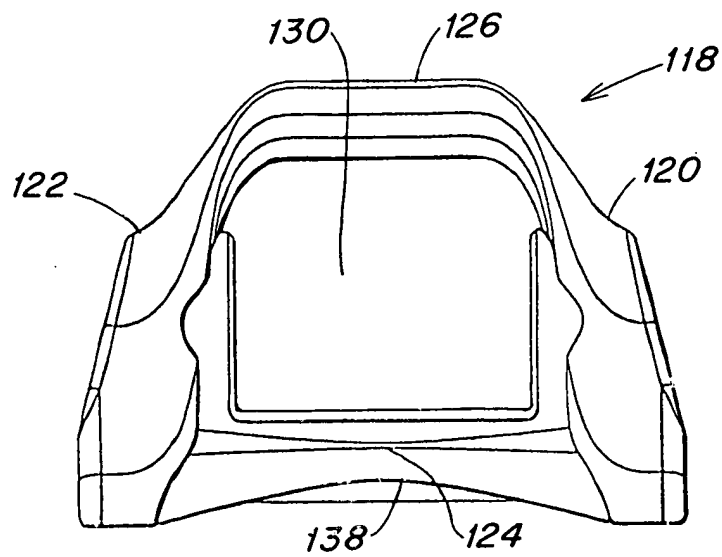

**FIG. 8**

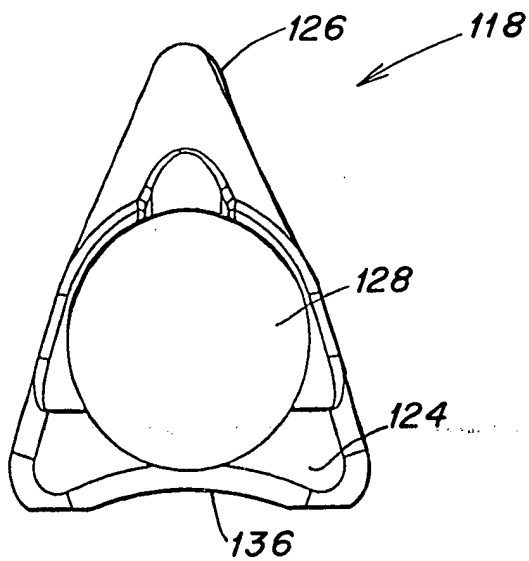

**FIG. 9**

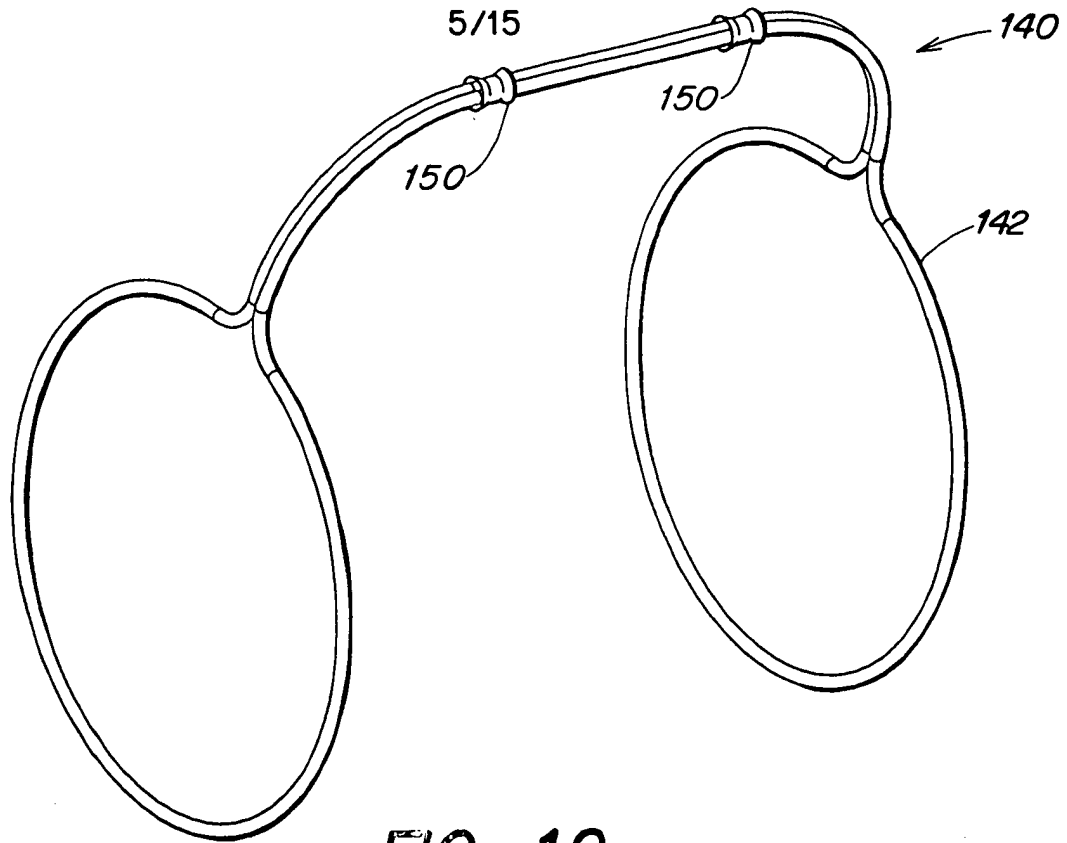


FIG. 10

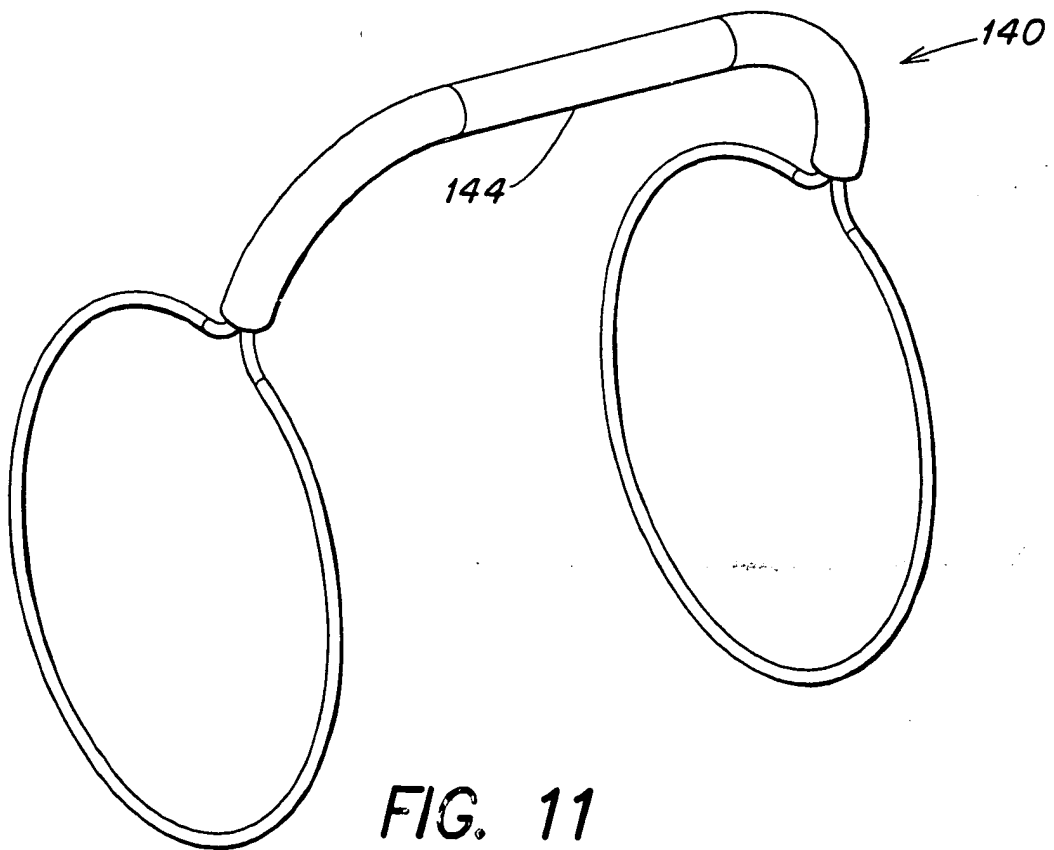


FIG. 11

6/15

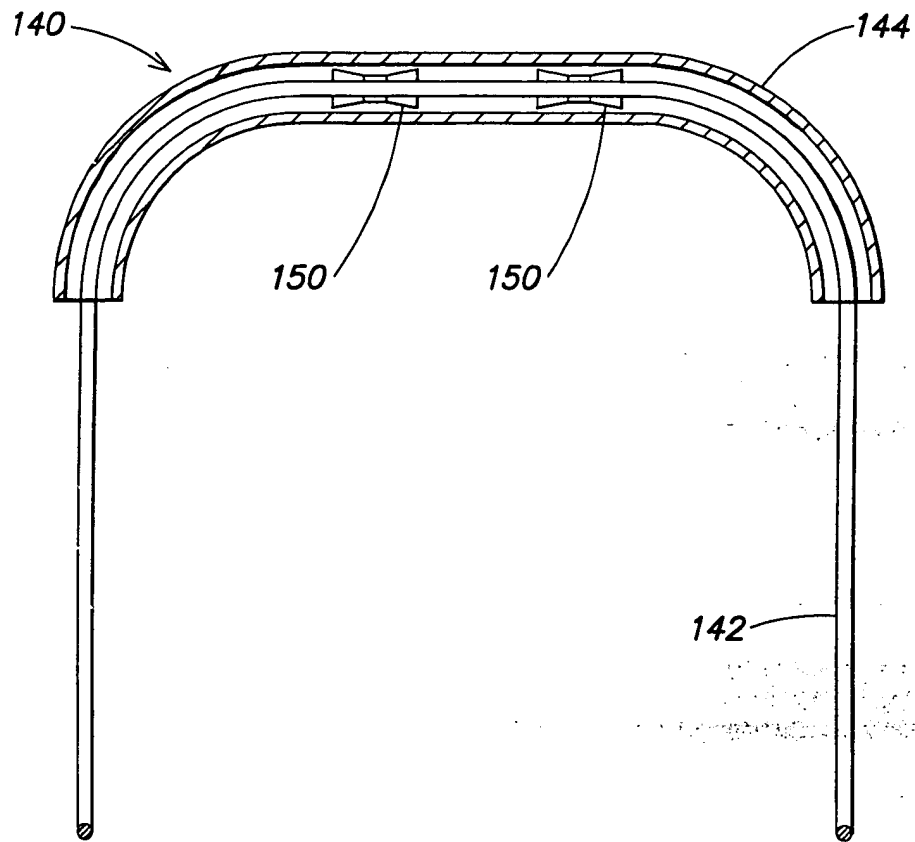


FIG. 12

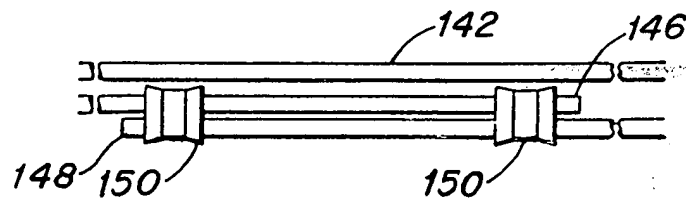


FIG. 13

# RADIOGRAPHIC CAMERA

Steven J. Grenier

09/687,554

Sheet 7 of 15

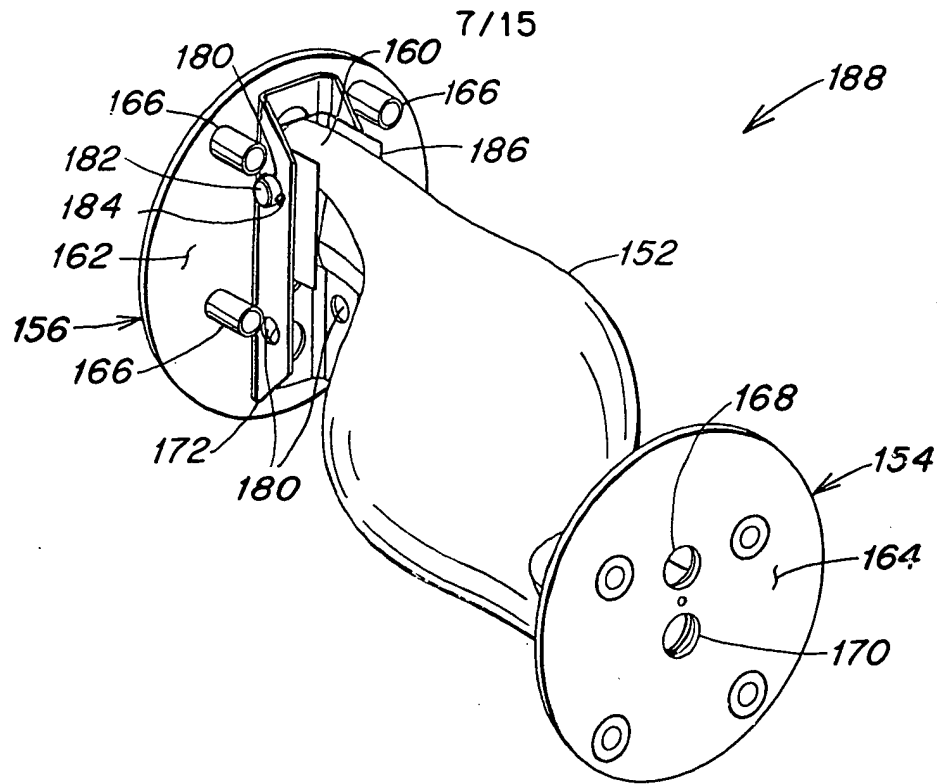


FIG. 14

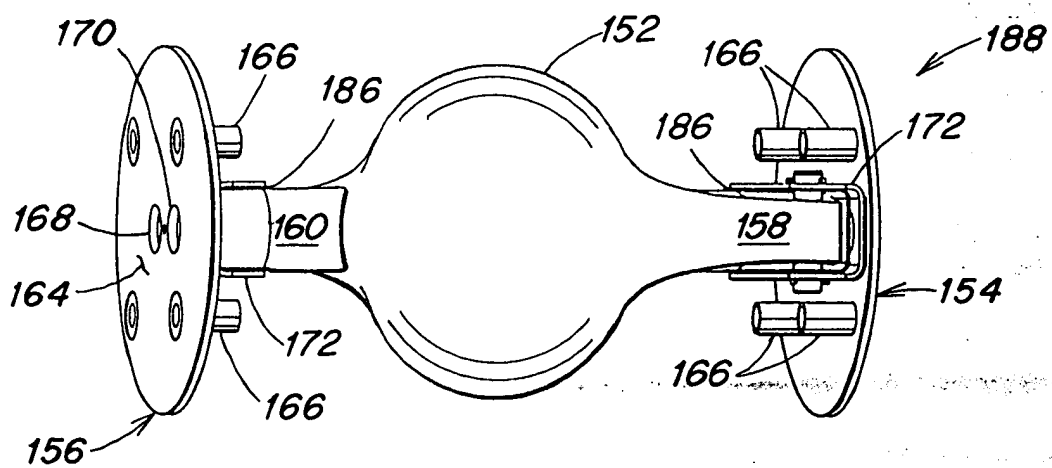


FIG. 15

8/15

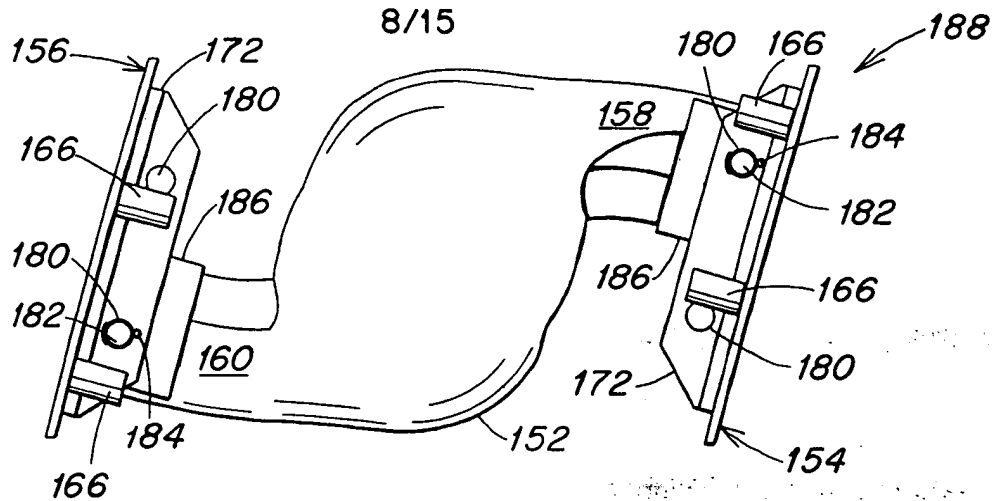


FIG. 16

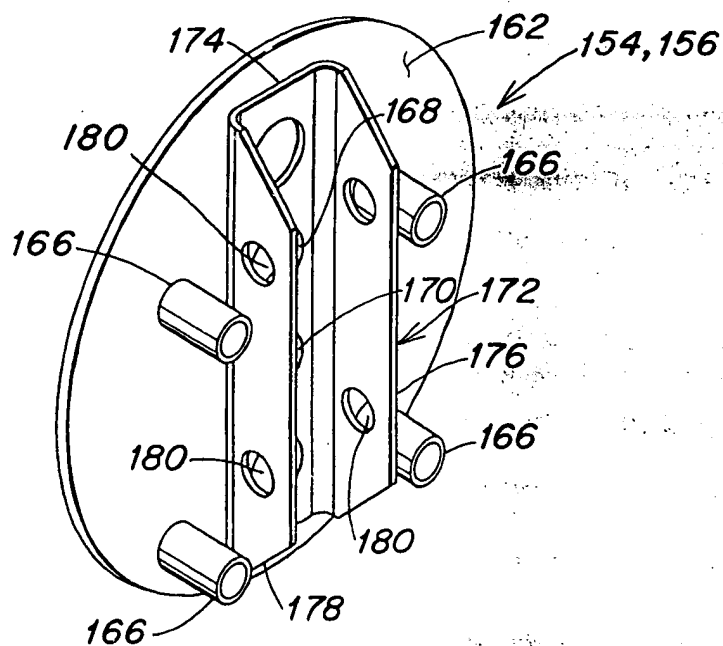


FIG. 17

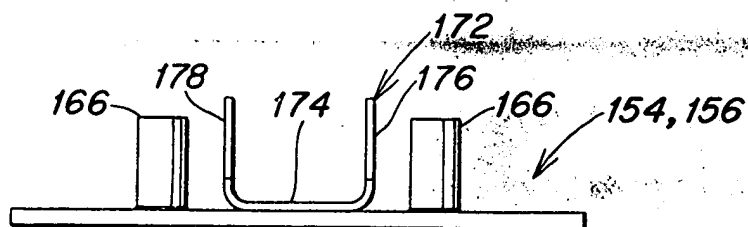


FIG. 18

RADIOGRAPHIC CAMERA

Steven J. Grenier

09/687,554

Sheet 9 of 15

9/15

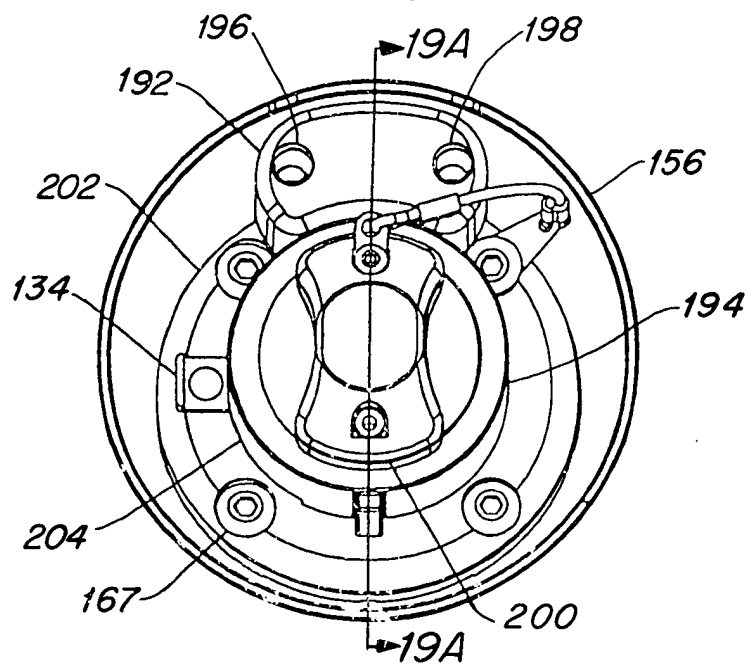


FIG. 19

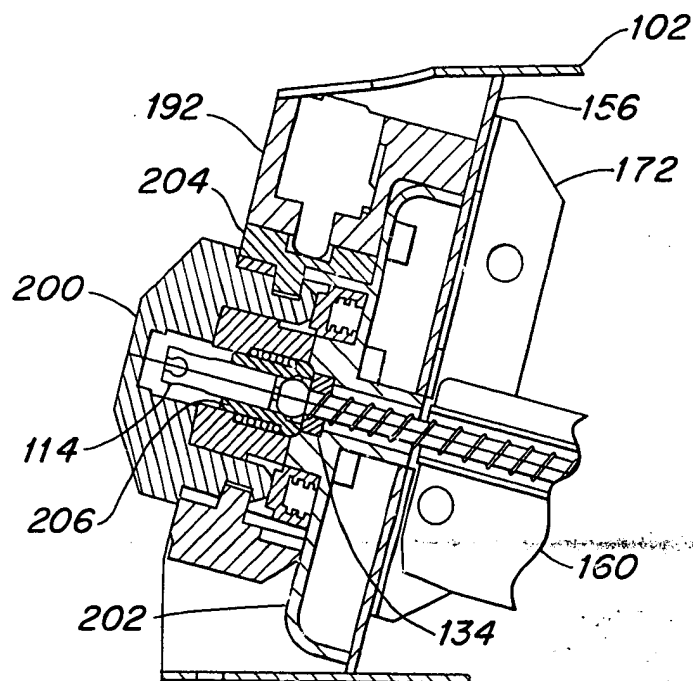


FIG. 19A

10/15

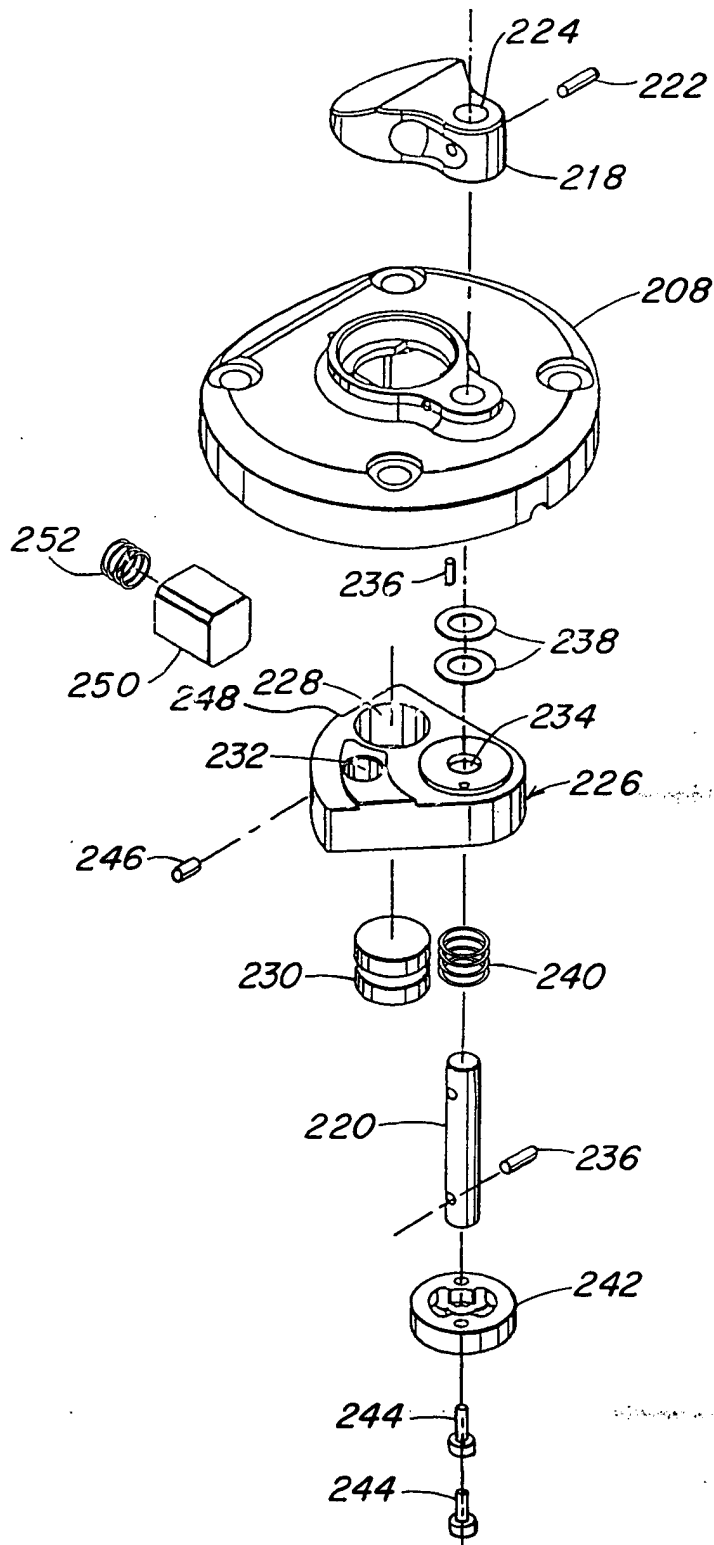


FIG. 20

# RADIOGRAPHIC CAMERA

Steven J. Grenier

09/687,554

Sheet 11 of 15

11/15

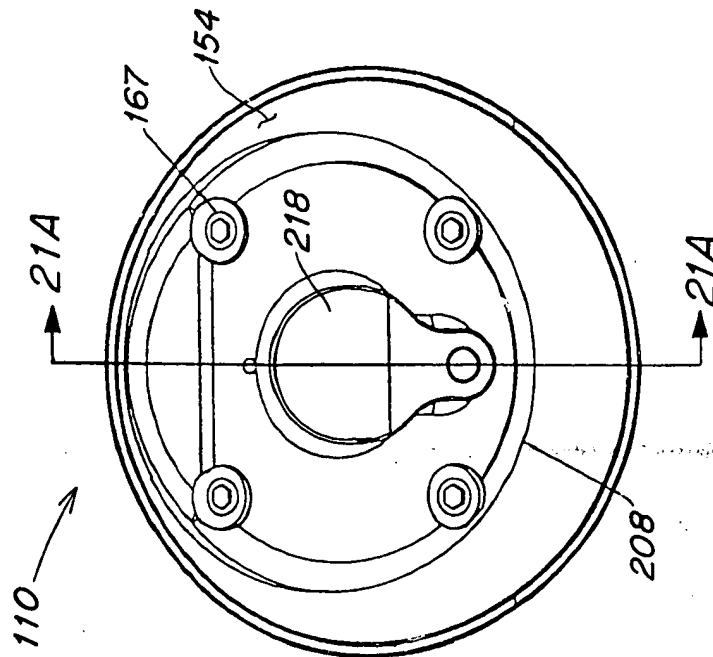


FIG. 21

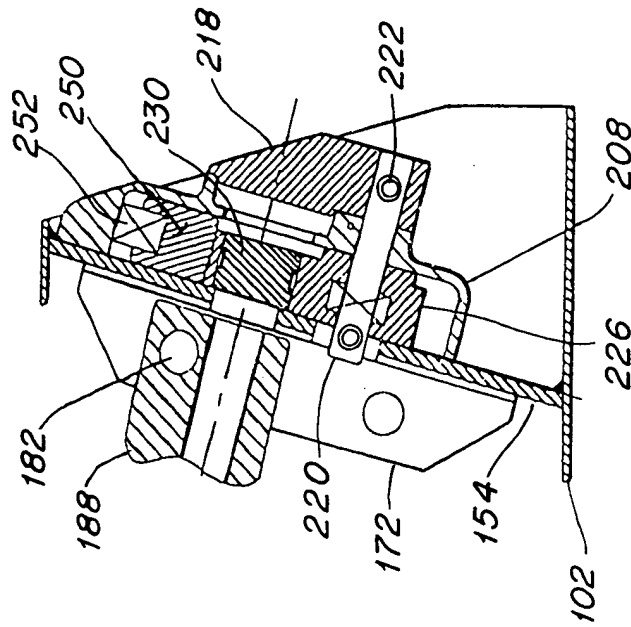


FIG. 21A

12/15

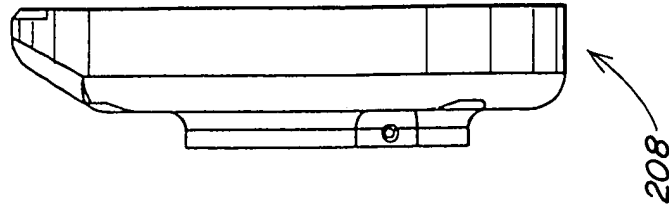


FIG. 24

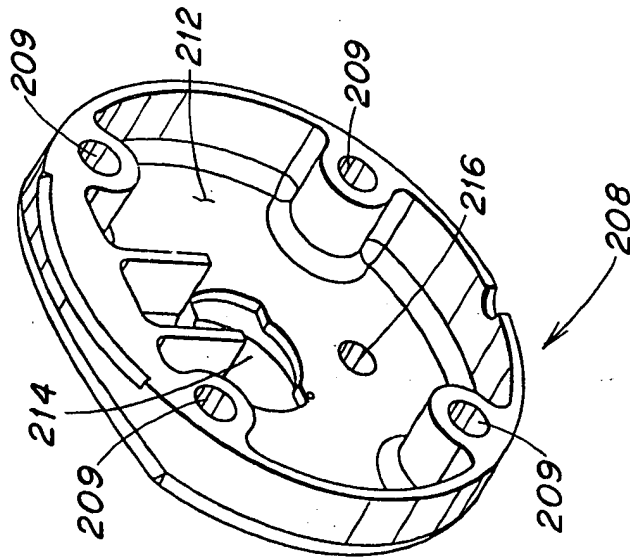


FIG. 23


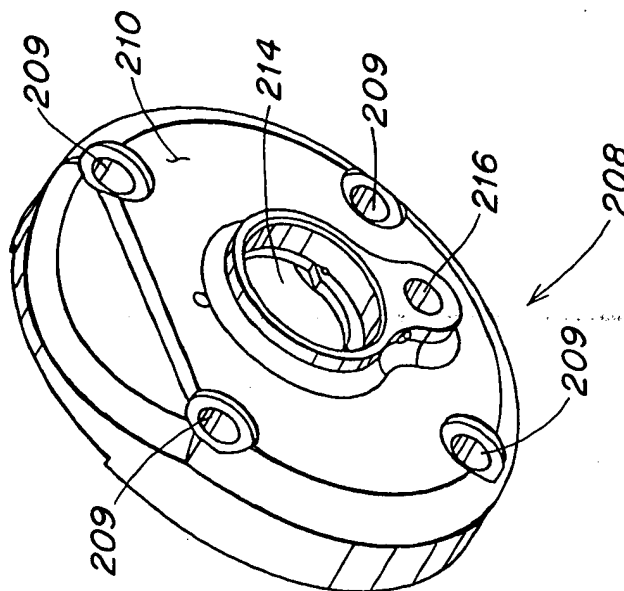



FIG. 22

13/15

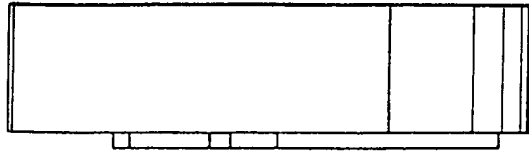


226

FIG. 27

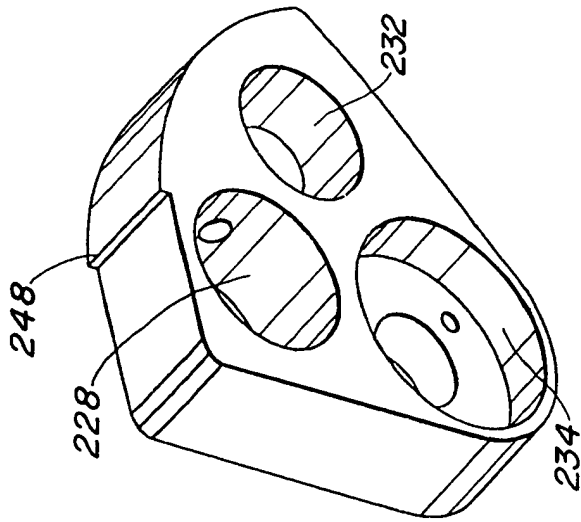

226

FIG. 26

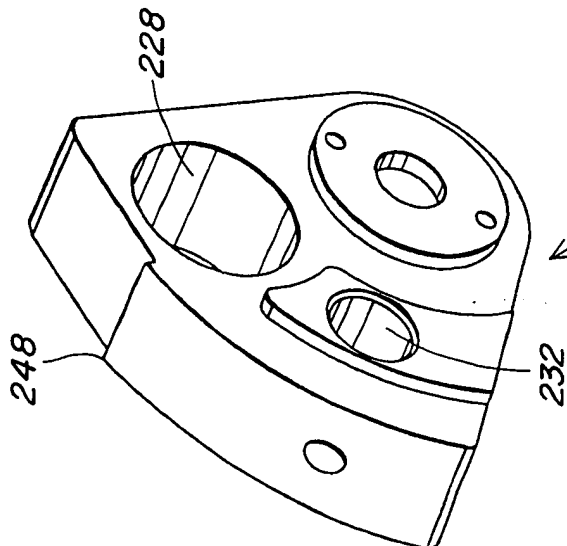

226

FIG. 25

15/15

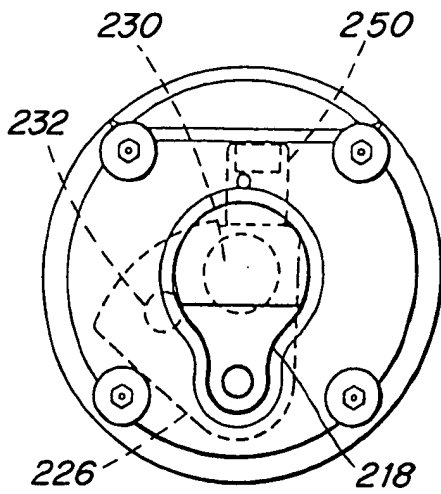


FIG. 31A

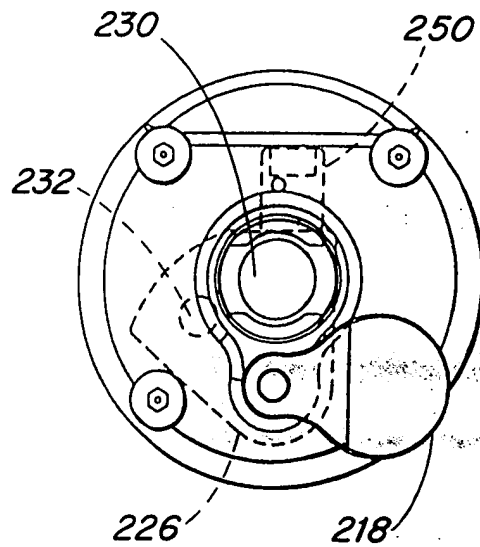


FIG. 31B

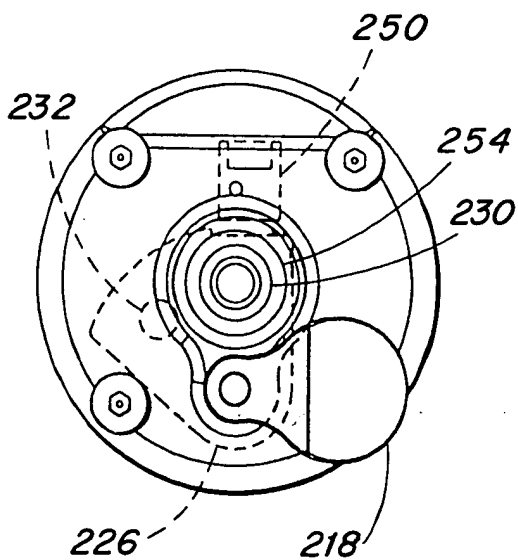


FIG. 31C

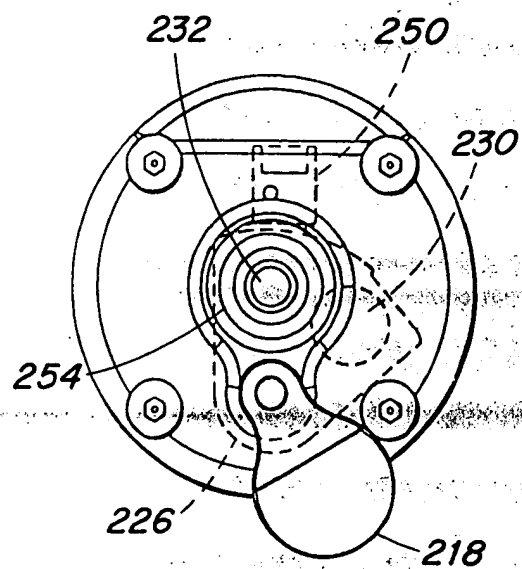


FIG. 31D